

SPHERO™ Flow Cytometry Nano Fluorescent Size Standard Kit

- Consists of fluorescent beads with 4 different diameters from 220nm to 1.33µm
- Designed to characterize microparticles (MPs, 0.5-0.9µm), aquatic bacteria (0.2-0.6µm), and platelets (0.9-3µm)
- Used to define optimal settings for MP analysis in new cytometers with increased Forward Scatter sensitivity
- Provides a submicron size standardization tool for flow cytometers
- An additional 130nm population is available as Catalog Number NFPPS-0152-5

Particle Type and Surface	Size, µm	Catalog No.	Unit
Nano Fluorescent Size Standard Kit, Flow Cytometry Grade, Yellow, 10 ⁶ /mL	0.1-0.3 µm, 0.4-0.6 µm, 0.7-0.9 µm, & 1.0-1.9 µm	NFPPS-52-4K	4x5 mL
Nano Fluorescent Size Standard, Flow Cytometry Grade, Yellow, 10 ⁶ /mL	0.05-0.15 µm,	NFPPS-0152-5	5 mL

Figure 84 SSC vs FITC Dot Plot using SSC trigger for Cat. No. NFPPS-4K, Lot AC01 on a Stratadigm S1400.

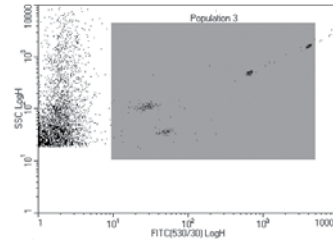


Figure 85 Dot Plots and Histograms of Cat. No. NFPPS-4K, Lot AC01, Peak 1, 0.22µm on a BD LSR2.

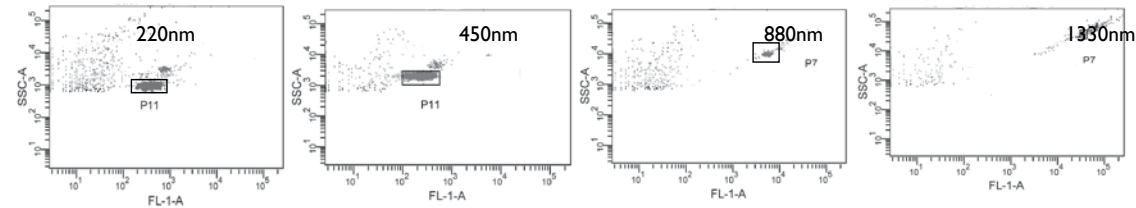


Figure 86 Cat. No. NFPPS-4K & NFPPS-0152-5 on a Beckman Coulter Cyan ADP

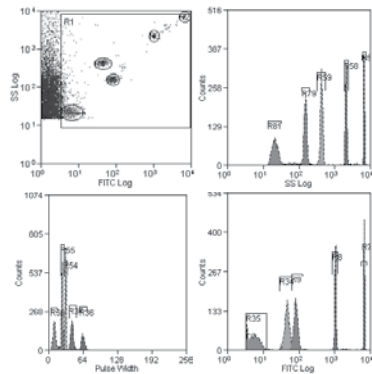


Figure 87 Dot Plots of Cat. No. NFPPS-4K, Lot AC01, on a Beckman Coulter XL.


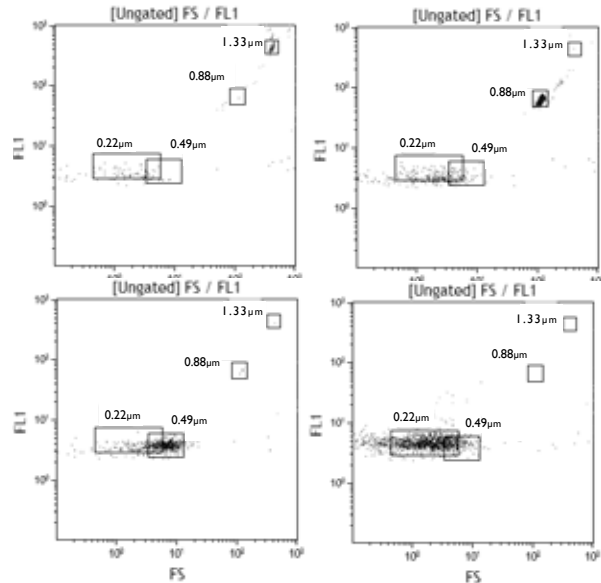


Figure 88 Cat. No. NFPPS-4K on a BD Fortessa X-20

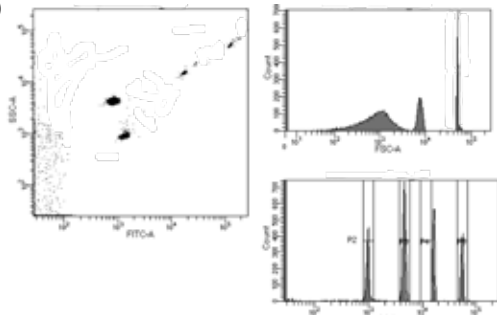

Flow Cytometry Particles - Nano Size Standard